

SENTINEL LYMPH NODE BIOPSY BY A HIGH T_c SQUID

Saburo Tanaka, Hajime Ota, Yoichi Kondo and Yukiko Matsuzawa

*Ecological Engineering, Toyohashi University of Technology, 1-1 Hibarigaoka Tempaku-cho
Toyohashi Aichi 441-8580, Japan*

Yasuhiro Tamaki and Shinzaburo Noguchi

*Department of Surgical Oncology, Biomedical Research Center Osaka university Graduate School
of Medicine, 2-2-E10 Yamadaoka, Suita, Osaka 565-0871, Japan*

The performance of a lymph node detection system used with a high T_c superconducting quantum interference device (SQUID) was investigated. The signal from the particles was dependent on the frequency of the magnetic field. This result suggested that the polarization is due to not only the alignment of the dipole moments but also the physical rotation of the particles.

INTRODUCTION

We have recently proposed the application of a high- T_c superconducting quantum interference device (SQUID) to the newly developed surgical technique of sentinel lymph node biopsy. Axillary lymph-node dissection is an important procedure in the surgical treatment of breast cancer. However, in the early diagnosis stage, the number of dissections in which axillary nodes are free of disease is apt to be increased. These treatments lead to some problems such as a lymph edema and a sensory neuropathy in the patient. The sentinel node biopsy is a kind of test to investigate whether the sentinel node, which initially receives malignant cells from a breast carcinoma is disease-free or not. If the sentinel node is free of disease, you can leave the rest of the lymph-nodes because of no concern for progression. This biopsy is based on the hypothesis that if the first lymph node (sentinel node) is free of disease, the second and the rest of the nodes must be negative. Two methods which detect the sentinel node have been developed and reported to date¹⁻³. One is a kind of radio guide, which uses a gamma detector and a radio isotope such as technetium labeled sulfur colloid. After injecting the isotope into a breast lesion, the sentinel lymph node will be identified by the gamma detector. Then the sentinel node is excised and examined. In this method the sentinel lymph-node is successfully identified with 94.4% accuracy¹. Though the predictability of this method is extremely high, radiation exposure is inevitable for medical staff. The other method uses a blue dye; a surgeon identifies the sentinel lymph-node with his naked eye. With this method the predictability is still 70% accurate².

Therefore we propose a localization system combined with a high sensitivity superconducting quantum interference device (SQUID) magnetometer and ultra-small

iron oxide particles. The system we are proposing is shown in Fig. 1. The particles would be injected into the breast; and the high- T_c SQUID is used as a sensing detector for the particles. This method has some advantages: no radiation exposure and an accurate identification because of the visible color of the particles themselves. For this application, the SQUID magnetic sensor should identify the location of the small quantity of particles under the sensor. Although a SQUID biosusceptometry system has been reported⁴, it is very difficult to detect the location because of the small quantity. Detection methods of small magnetic particles with a SQUID immunoassay, which can be also applied to our detection system, have been proposed in several groups⁵⁻⁷. Even if the particles are made of iron oxide, if their size becomes too small, they show superparamagnetic properties. Therefore, some magnetic field should be applied to the particles for detection because they have almost no permanent magnetic dipole at room temperature. Koetitz *et.al.* applied a pulse field to the particles and then measured the field decay from the particles in the range of ms. Enpuku *et.al.* measured the field from the particles under a DC magnetic field. For the work described here, we measured the field from the particles under an AC magnetic field.

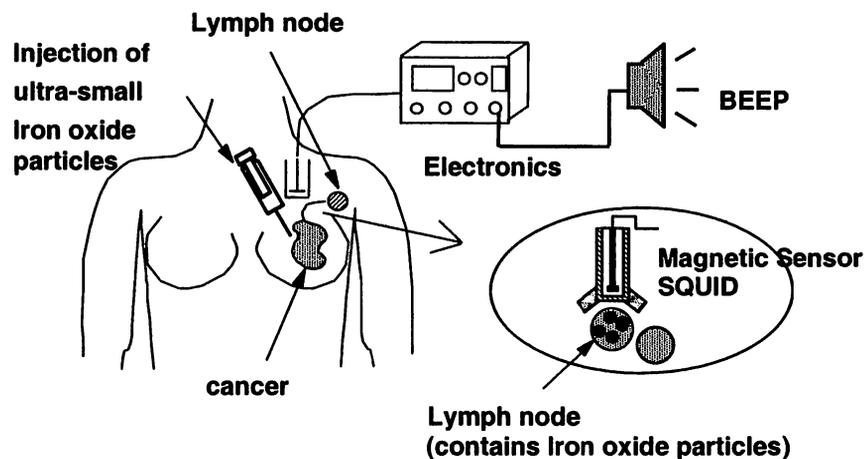


Fig. 1. The system diagram of the sentinel-node biopsy using high T_c SQUID, which we are proposing. The particles would be injected into the breast; and the high- T_c SQUID is used as a sensing detector for the particles. This method has an advantage of no radiation exposure.

We have already reported the results of preliminary study using particles dispersed liquid in a tube⁸. In this paper, we discuss about a magnetic field frequency dependence of the SQUID signal.

EXPERIMENTAL SETUP

The schematic diagram of the system is shown in Fig. 2. The SQUID is made of $Y_1Ba_2Cu_3O_{7-y}$ thin film. The junctions utilized in the SQUID are of the step-edge type. The washer size of the SQUID is about $2.5 \times 2.5 \text{ mm}^2$ and the effective area is 0.11 mm^2 . The SQUID was operated in a flux-locked loop. The magnetic flux noise in the white noise region was about $30 \mu\phi_0/\text{Hz}^{1/2}$.

The cryostat was specially designed for a SQUID microscope. The SQUID was located inside a vacuum and separated by a $50\ \mu\text{m}$ thick quartz window. A more detailed description can be found elsewhere⁹. Two coils (Helmholtz type) were mounted just above the SQUID microscope^{10,11}. A fine polytetrafluoroethylene tube with an inner dimension of 0.85-0.95 mm dia., which conveys small particles, was threaded into the coils. A motor driven syringe pump was employed to convey the particles by pushing air inside the tube. A sinusoidal AC current with a frequency of 5Hz - 100Hz was directed to the coils; the magnetic field generated from the coil was modulated by the frequency. The modulated signal associated with the particle motion was then demodulated by the lock-in-amplifier. The lock-in-amplifier consists of a phase sensitive detector, a phase shifter and a low-pass filter¹². The use of the lock-in-amplifier is a crucial point to obtain a good resolution in the system. The SQUID position was carefully adjusted before measurement, so that the SQUID output signal without particles became zero.

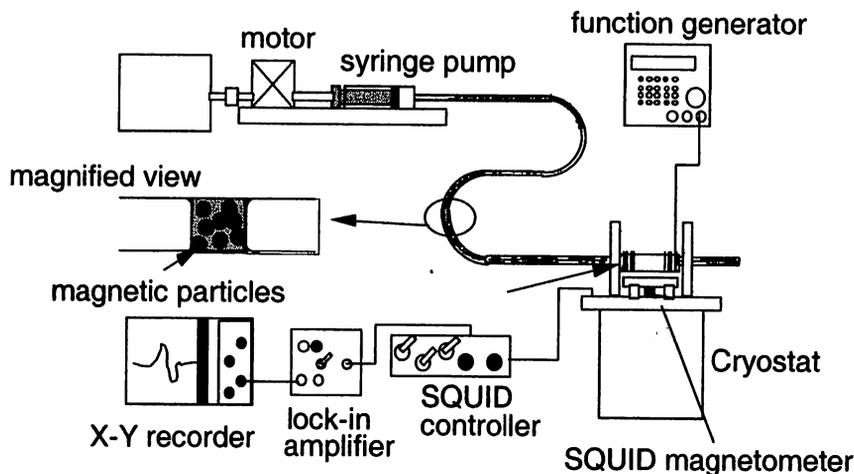


Fig. 2. Schematic diagram of the system for the feasibility test. A pair of coils were mounted just above the SQUID cryostat. External ac magnetic field was applied by the coils. A motor driven syringe pump was employed to push the magnetic particle sample inside a thin tube. The modulated signal associated with the particle motion was demodulated by the lock-in amplifier.

After adjusting the SQUID, the system was ready to measure magnetic field from the particles. We used ultra-small particles from Meito Sangyo Co., Ltd. Similar particles are used as a magnetic resonance imaging (MRI) contrast agent. The core of the particle is iron oxide Fe_3O_4 (magnetite) which is coated with an alkali-treated dextran. The average core diameter was 11nm, which was measured from the X-ray diffraction pattern using Scherrer's equation¹³. The averaged diameter of the coated particles was 100nm. The particles had superparamagnetic properties. The particles were supplied in the form of an aqueous magnetic fluid. The original fluid contained 5.9 mg/ml of iron. If we suppose $5.2\ \text{g}/\text{cm}^3$ as the specific gravity of the core, we can estimate the weight of the mono-particle as $3.6 \times 10^{-18}\ \text{g}$ and the total number of particles in the original solution as $1.5 \times 10^{16}/\text{ml}$. The original fluid was diluted with distilled water to have the desired concentrations. Then the fluid was swept in the fine

tube with the scan speed of 0.33-1.1 mm/sec under an AC magnetic field of 9×10^{-5} to 7×10^{-4} T (peak to peak value).

RESULT AND DISCUSSIONS

We performed all of the measurements in a magnetically shielded room with a shielding factor of -50 dB at 0.1 Hz. We investigated the detectable weights of the iron. The SQUID signal was proportional to the weight of the iron in the fluid. At a distance of 40 mm, the minimum detectable weight was $1.6 \mu\text{g}$. When the distance was decreased to 1 mm, this decreased to 360pg^8 .

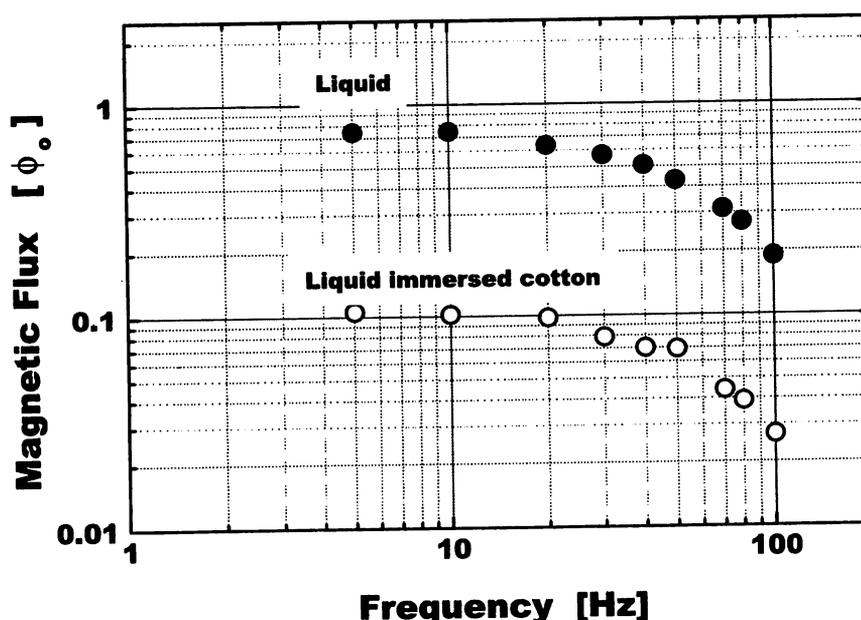


Fig. 3. Frequency dependence of the output signal. The modulation frequency of the Helmholtz coil was changed from 5 Hz to 100 Hz. Closed circles show the results from liquid sample. Open circles show the results from liquid with a piece of cotton.

Then we measured the frequency dependence of the output signal. The sample consisted of iron particles of $2.4 \mu\text{g}$ and distilled water of $4.4 \mu\text{l}$. The modulation frequency of the Helmholtz coil was changed from 5 Hz to 100 Hz. The results are shown in Fig. 3 (solid circles). The signal from the lock-in amplifier decreased with the increase of frequency in the region of more than 10 Hz. The results suggested that the alignment of the dipole moments or the rotation of the particles is not synchronized with the frequency. Therefore we immersed a piece of cotton with the liquid sample. The content of the iron and the volume of the liquid were as same as the former experiment. In this sample, the rotation of the particles should be restricted by existence of the cotton though it was not perfectly. The frequency dependence was measured using this sample. The results were shown in Fig. 3 (open circles). The signal was one order smaller than that of the liquid sample in all the frequency; this is because of the restriction of the particle's rotation. Although further experiments are needed

to clarify this phenomenon⁷, not only the alignment of the dipole moments but also the physical rotation of the particles is contributed to the polarization. Therefore the lower frequency should be chosen in the system.

CONCLUSION

We have demonstrated the possibility of realization of a nanoparticle detection system used with a high- T_c SQUID, which is useful for sentinel lymph node biopsies. The ultra-small iron oxide particles of 360 pg in weight of iron could be detected with a spacing of 1mm. The signal from the particles was dependent on the frequency of the magnetic field. This result suggested that the polarization is due to not only the alignment of the dipole moments but also the physical rotation of the particles.

ACKNOWLEDGMENTS

This work was partially supported by a grant-in Aid for Science Research (B) from the Ministry of Education, Culture, Sports, Science and Technology and also supported by THE SAGAWA FOUNDATION FOR PROMOTION OF CANCER RESEARCH.

REFERENCES

1. U. Veronesi, G. Paganelli, V. Galimberti, G. Viale, S. Zurrída, M. Bedoni, A. Costa, C. de Cicco, J. G. Geraghty, A. Luni, V. Sacchini and P. Veronesi, *The Lancet* **349**, 1864 (1997).
2. A. E. Giuliano, D. M. Kirgan, J. M. Guenther and D. L. Morton, *Ann Surg.* **220** , 398 (1994).
3. C. E. Cox, S. P. Pendas, J. M. Cox, E. Joseph, A. R. Shons, T. Yeatman, N. N. Ku G. H. Lyman, C. Berman, F. Haddad and D. S. Reintgen, *Annals of Surgery* **227**, 645 (1998).
4. R. Engelhardt, R. Fisher, P. Nielsen, and E. E. Gabbe, *Proc. of 10th International Conference on Biomagnetism*, 187 (1996).
5. R. Koetitz, H. Matz, L. Trahms, H. Koch, W. Weitschies, T. Rheinlaender, W. Semmler and T. Bunte, *IEEE Trans. Appl Supercond.* **7**, 3678 (1997).
6. K. Enpuku, T. Minotani, T. Gima, Y. Kuroki, Y. Itoh, M. Yamashita, Y. Katakura and S. Kuhara, *Jpn. J. Appl. Phys.* **38** , L1102 (1999).
7. Y.R.Chemla, H.L.Grossman, Y.Poon, R.McDermott, R.Stevens, M.D.Alper and J.Clarke, *Proc. The National Academy of Sciences* **97**, 14268 (2000).
8. S.Tanaka and A.Hirata, Y.Saito. T.Mizoguchi, Y.Tamaki, I.Sakita and M.Monden, *IEEE Trans. on Applied Supercond.* **11**, 665 (2001).
9. S. Tanaka, O. Yamazaki, R. Shimizu and Y. Saito, *Jpn. J. Appl. Phys.* **38**, L505 (1999).
10. S.Kumar, R.Matthews, S.G.Haupt, D. K. Lathrop, M. Takigawa, J.R.Rozen, S.L.Brown and R.H.Koch, *Appl. Phys. Lett.* **70**, 1037 (1997).

11. K. Schlenga, R. McDermott, John Clarke, R.E. de Souza, A.Wong-Foy and A.Pines, *Appl. Phys. Lett.* **75**, 3695 (1999).
12. A. Pasquarelli, C. Del. Gratta, S. Della Penna, S. Di Luzio, V. Pizzella, G. L. Romani, *Phys. Med. and Biol.* **41**, 2533 (1996).
13. M. Hasegawa, S. Maruno, T. Kawaguchi and T. Moriya, *Proc. 6th Int. Conf. Ferrites, Tokyo and Kyoto*, 1007 (1992).